

Fig. 1

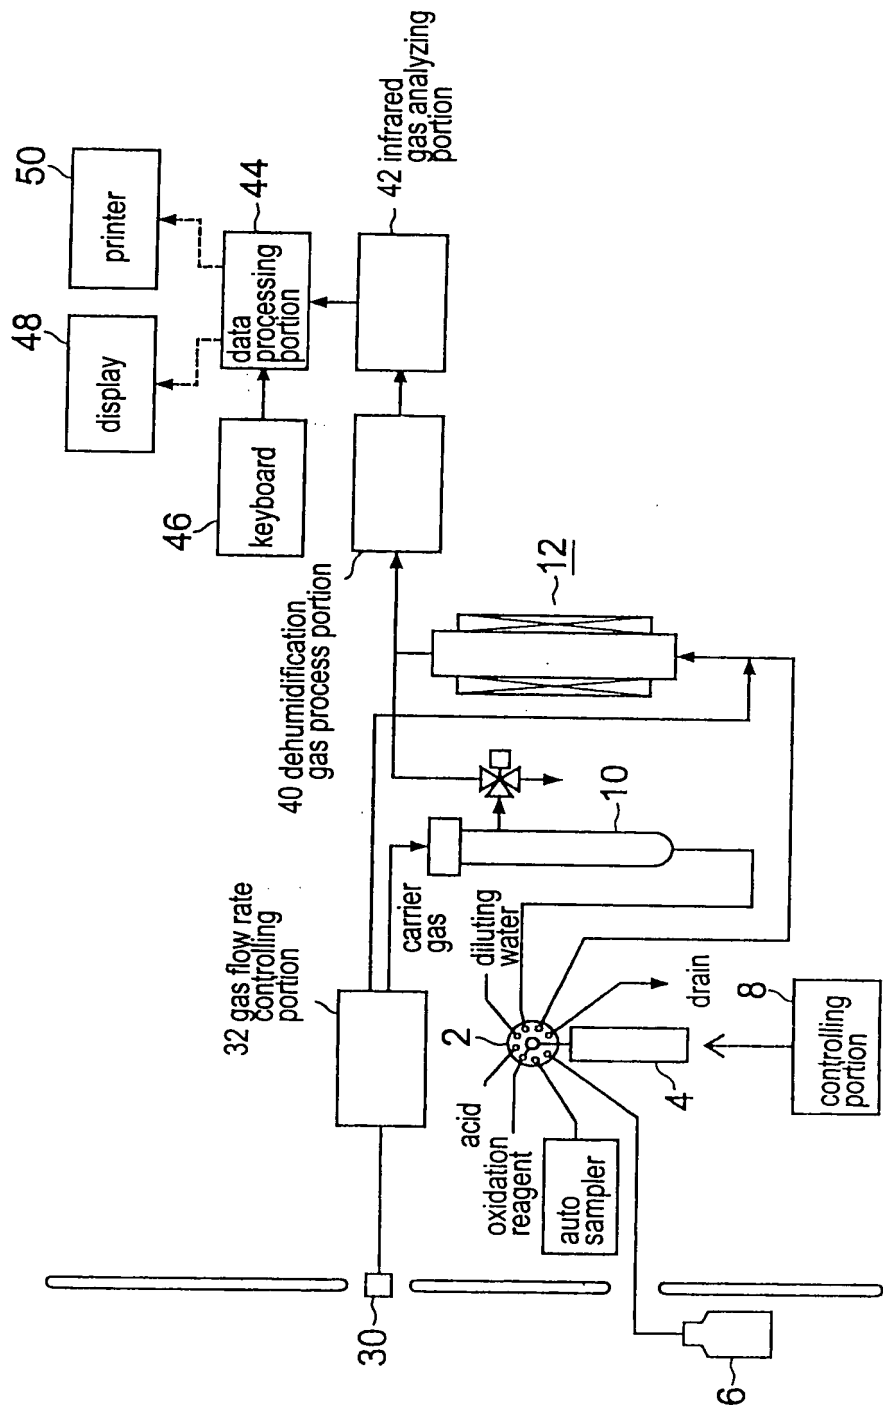


Fig. 2

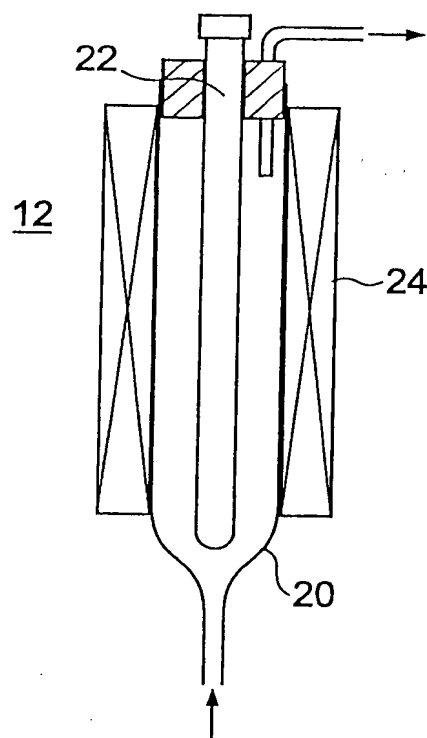


FIG. 2 is a cross-sectional view of the device.

Fig. 3

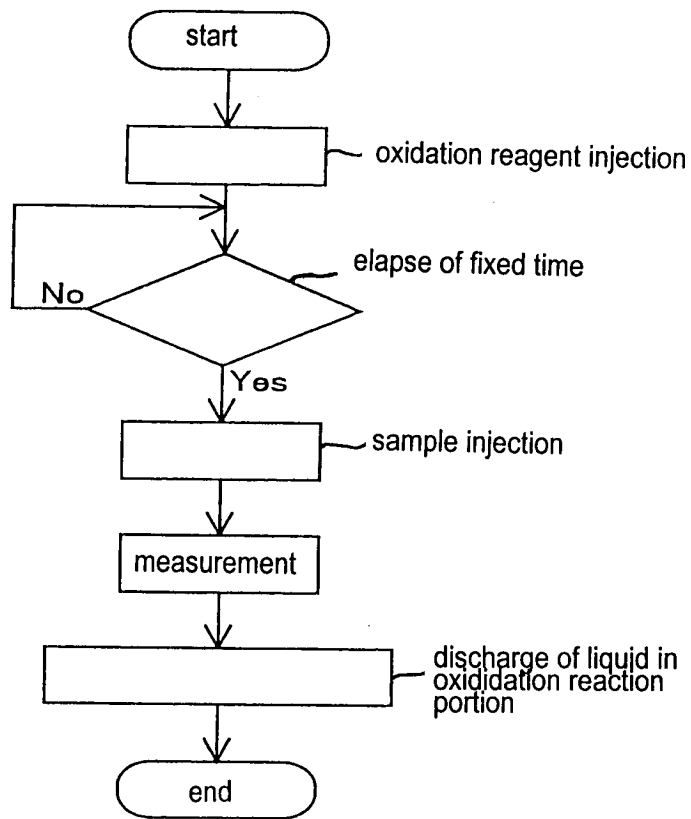


Fig. 4

